ANALIZA BIAŁEK

Scan for verify

100018241

Laboratory of Analysis

Client: https://roidteam.net/
Order number: 100018241
Name: HILMA BIOCARE SOMATROPIN
Number of samples: 1 wstrzykiwacz

Batch number: 608H92/39
Receive date: 2026-09-09
Start date: 2026-09-11
End date: 2026-09-16

Sample identification

Substance	Method of taking a sample	Form
hGH	Sample provided by customer	Transparent liquid in a syringe

Results

Substance	Sample name	Content	Purity
hGH	HILMA BIOCARE SOMATROPIN 30MG	9,46mg/ml (28,42 I.U.) 28,39mg/3ml	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its content, when compared to the reference chromatogram, is 9,46mg/ml (28,42 I.U.) 28,39mg/3ml. Height the measurement error is +-0,05mg. The actual state of the sample sent before the test is presented on the photo below.

Photo of the test sample



Password

CI6499WW

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Du□ska 9, 54-427 Wrocław
Budynek DELTA


Lab technician:
Analysis and research specialist
mgr Arkadiusz Zaj□c

ANALIZA BIAŁEK

Scan for verify

100018241

Chromatogram

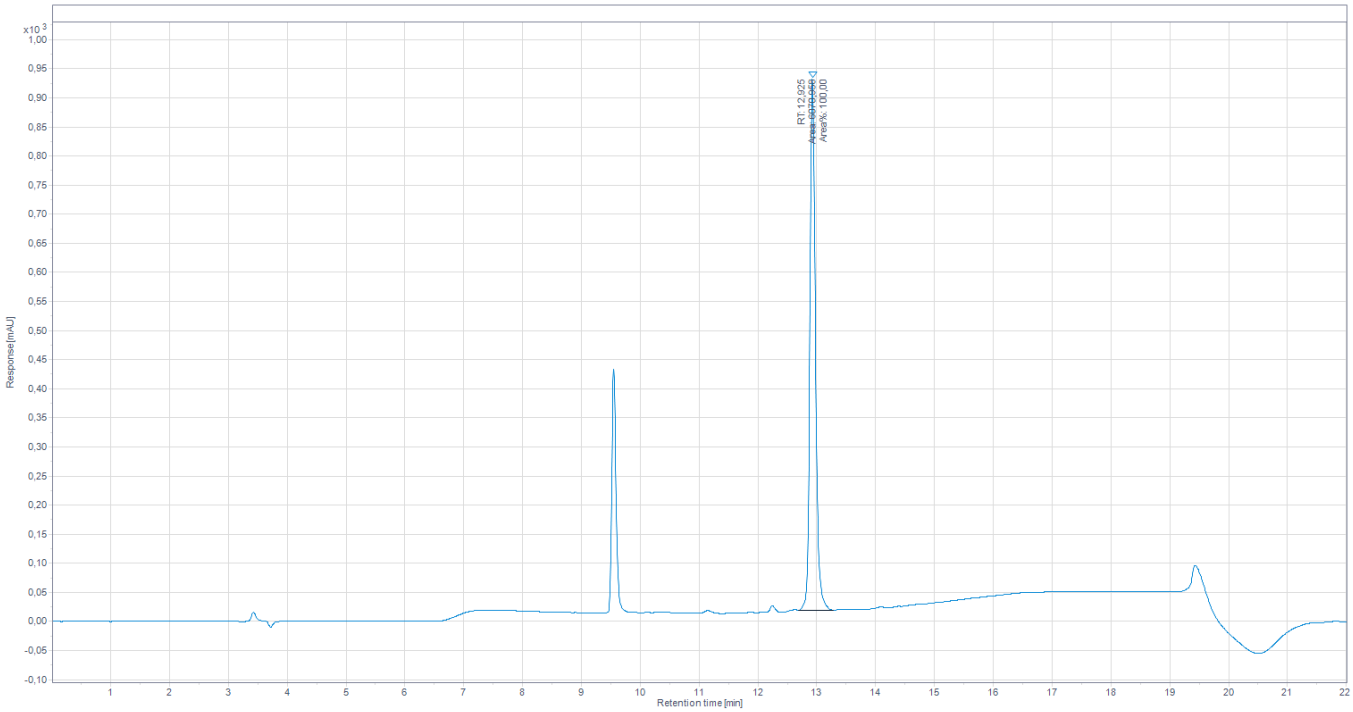

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	60%	40%
2min	60%	40%
27min	5%	95%
30min	5%	95%

Password

CI6499WW

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Du□ska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zaj□c